

SYSTEMATIC REVIEW

Which clinical and laboratory procedures should be used to fabricate digital complete dentures? A systematic review



Khaing Myat Thu, BDS, DipDSc, PhD,^a Pedro Molinero-Mourelle, Dr med dent, PhD,^b
Andy Wai Kan Yeung, BDS, PhD,^c Samir Abou-Ayash, Prof, Dr med dent,^d and
Walter Yu Hang Lam, BDS, MDS(Pros), AdvDipProsth, FHKAM, FCDSHK, MFDS (RCSEd), MFDS (RCPSG), FDS
(RCSEd), FDS (RCPSG), MPros RCSEd, FRACDS^e

Computer-aided design and computer-aided manufacturing (CAD-CAM) system for complete denture fabrication has greatly advanced, offering benefits such as fewer clinical visits with shorter chairtime,¹⁻³ better material properties,⁴ and cost savings.^{2,5,6} Digital denture technology began as early as 1994,⁷ with earlier techniques⁷⁻⁹ making edentulous impressions before the intraoral scanning of edentulous jaws was proposed.¹⁰ Most earlier digital dentures followed conventional denture techniques, but gradually a fully digital workflow was adopted.^{11,12} Furthermore, the recent development of materials and technology has made 3D printing a suitable option for digital dentures.¹³

The digital workflow for the fabrication of complete

ABSTRACT

Statement of problem. Digital workflows for digital complete denture fabrication have a variety of clinical and laboratory procedures, but their outcomes and associated complications are currently unknown.

Purpose. The purpose of this systematic review was to evaluate the clinical and laboratory procedures for digital complete dentures, their outcomes, and associated complications.

Material and methods. Electronic literature searches were conducted on PubMed/Medline, Embase, and Web of Science for studies published from January 2000 to September 2022 and screened by 2 independent reviewers. Information on digital complete denture procedures, materials, their outcomes, and associated complications was extracted.

Results. Of 266 screened studies, 39 studies were included. While 26 assessed definitive complete dentures, 7 studies assessed denture bases, 2 assessed trial dentures, and 4 assessed the digital images only. Twenty-four studies used border molded impression technique, 3 studies used a facebow record, and 7 studies used gothic arch tracing. Only 13 studies performed trial denture placement. Twenty-one studies used milling, and 17 studies used 3D printing for denture fabrication. One study reported that the retention of maxillary denture bases fabricated from a border-molded impression (14.5 to 16.1 N) was statistically higher than the retention of those fabricated from intraoral scanning (6.2 to 6.6 N). The maximum occlusal force of digital complete denture wearers was similar across different fabrication procedures. When compared with the conventional workflow, digital complete dentures required statistically shorter clinical time with 205 to 233 minutes saved. Up to 37.5% of participants reported loss of retention and up to 31.3% required a denture remake. In general, ≥1 extra visit and 1 to 4 unscheduled follow-up visits were needed. The outcomes for patient satisfaction and oral health-related quality of life were similar between conventional, milled, and 3D printed complete dentures.

Conclusions. Making a border-molded impression is still preferred for better retention, and trial denture placement is still recommended to optimize the fabrication of definitive digital complete dentures. (J Prosthet Dent 2024;132:922-938)

This research did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors. The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper. Presented at the International Association for Dental Research (IADR) General Session 2022, Chengdu, PR China, April 24, 2022 (Titled: A Systematic Review of Procedures for Digital Complete Dentures).

^aSenior Research Assistant, Restorative Dental Sciences, Faculty of Dentistry, The University of Hong Kong, Hong Kong Special Administrative Region, PR China.

^bResearch Assistant, Department of Reconstructive Dentistry and Gerodontology, School of Dental Medicine University of Bern, Bern, Switzerland.

^cTutor in Oral and Maxillofacial Radiology, Applied Oral Sciences and Community Dental Care, Faculty of Dentistry, The University of Hong Kong, Hong Kong Special Administrative Region, PR China.

^dAssociate Professor, Department of Reconstructive Dentistry and Gerodontology, School of Dental Medicine, University of Bern, Bern, Switzerland.

^eClinical Assistant Professor in Prosthodontics, Restorative Dental Sciences, Faculty of Dentistry, The University of Hong Kong, Hong Kong Special Administrative Region, PR China.

Clinical Implications

Extra clinical visits may be needed to address the problems of retention, jaw relationship errors, and poor esthetics of digital complete dentures, emphasizing the need for making an optimal impression, recording correct jaw relationships, and trial denture placement.

dentures has been evaluated in clinical studies, in which time and costs,^{2,5,6} clinical outcomes,^{3,13,14} patient-reported outcomes,¹³⁻¹⁷ and denture complications¹⁸⁻²⁰ have been investigated. Although some of these studies reported favorable results and edentulous patients may have benefited by attending fewer clinical visits than with conventional dentures,¹ complications with digital complete dentures such as extra visits and clinical time for adjustment, repair, or even remake have been reported.^{16,18-21}

Edentulous jaws can be captured by making an impression or intraoral scanning, and denture bases can be fabricated by milling or 3D printing. The outcomes,²² associated complications,²¹ or both^{4,23} of digital complete dentures have been evaluated.²⁴ However, reviews of denture fabrication procedures and their outcomes or associated complications are lacking. Therefore, this systematic review aimed to evaluate clinical and laboratory procedures for fabricating digital complete dentures, their outcomes, and associated complications among published clinical studies. The research hypothesis was that the outcomes and complications of digital complete dentures would be associated with their clinical and laboratory fabrication procedures.

MATERIAL AND METHODS

This systematic review was conducted by following the Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) 2020 expanded format²⁵ and was registered on the PROSPERO International prospective register of systematic reviews (CRD42023393061). The review question "What outcomes or complications are associated with various clinical and laboratory procedures for the fabrication of digital complete dentures in previous clinical studies?" was designed by using a population, intervention, control, and outcomes (PICO) model: completely edentulous population, digital complete dentures intervention, conventional denture workflow as control, and all outcomes including complications associated with digital complete dentures. Two independent assessors (K.M.T., P.M.-M.) searched electronic literature related to digital complete dentures on PubMed/Medline, Embase, and Web of Science databases

from January 2000 to September 2022. Supplementary hand-searching on Google Scholar and tracing references of selected studies was used to identify any missing studies. Search terms and search queries are presented in [Supplementary Table 1](#) (available online).

The retrieved studies were first screened according to the relevance of titles and abstracts. The shortlisted studies were then assessed with full-text analysis in which the inclusion criteria were: clinical studies only, written in English, using subjective or objective measurements to assess the outcomes or associated complications. Studies written in other languages, those not related to clinical study, and studies other than original research articles such as case reports, short communications, commentaries, and reviews were excluded. Disagreements between assessors were resolved by discussion. The risk of bias in each study was assessed by an independent and calibrated assessor (K.M.T.). The screening process and data extraction were performed using a systematic review software program (Covidence; Veritas Health Innovation).

The data were extracted by the same assessors independently, and any differences were resolved through discussion. Extracted data from each study include details of the clinical and laboratory procedures of digital complete denture fabrication, number of dentures or specimens and denture materials, outcomes, associated complications, and maintenance needs. The frequency of use of each clinical and laboratory procedure and the complications were recorded. Evaluation of these data was categorized into clinical procedures, laboratory procedures and denture materials, and outcomes and associated complications.

RESULTS

A total of 1780 studies were screened for the relevance of title and abstract after the removal of duplicates. The shortlisted 266 studies were assessed for full text, and 39 studies ([Table 1](#)) were included for data extraction according to the eligibility criteria ([Fig. 1](#)). The assessment results for risk of bias for different study designs are presented in [Supplementary Tables 2 to 4](#), available online. Seven randomized controlled trials^{13,26-31} had fair to good quality, but 13 cohort studies^{1-3,20,32-40} and 3 other studies^{16,41,42} were considered poor quality. The remaining studies were also considered fair to good quality.

Among 39 included studies, 7 studies^{33,37,38,40,43-45} assessed denture bases, 2 studies^{8,36} assessed trial dentures, and 26 studies^{1-3,5,6,13-20,26-31,41,42,46-50} investigated definitive complete dentures, including 2 studies^{26,29} with implant overdentures (IOD). Four studies^{32,34,35,39} assessed digital scans of impression or edentulous jaws for

Table 1. Clinical studies with digital denture fabrication or digital analysis included^{1,2,3,5,6,8,13–20,26–50}

No.	Study	Study objects (or Examined specimens)	No. of digital dentures	Digital systems	Visits	Primary impression making	Positive impression making	Digitization of arch	Flow relationship record	Use of articulator mounting	Try-in placement	Clinical routine	Fabrication of definitive dentures	Denture occlusal scheme	Materials used for denture base	Maintenance needs before denture delivery	Follow-up or complaint
1	Inokoshi 2012 ¹	Wax CD	10	3D CAD program (CATIA VR D ₁ , 3D Systems, Formlabs, Shogun, Techbio logics, etc.)	NA	by duplicate denture	By wash molding without border (duplicate denture)	Scanned the duplicate fabricated wax denture (conventional dentures)	Using duplicate denture	Mechanical articulator (bush not specified)	Wax denture	NA	Only 3D printed trial dentures	Not specified	Ultra violet-based resin material (FullCure 720, Dyract Composites)	-Needed for rearrangement -Needed to re-fabricate	3D printed dentures showed inferior ability
2	Karuse 2013 ¹	CD Set	10 (Same as above study)	Mimic CAD software program	-	NA	NA	NA	Using old denture	Not specified	NA	NA	3D Printing	Not specified	Ultra violet-polymerized acrylic-based resin material	NA	NA
3	Katradyil 2015 ¹⁴	CD Set	15	Avantek	2	NA	Border-molded impression	Not specified	Avantek protocol	NA	NA	NA	Milling	Lingualized occlusion	Not specified	-Anterior open occlusal relationship -Lingualized occlusion to re-fabricate	6.6% of patients (anterior open relation)
4	Saponaro 2016 ¹⁵	CDs	50	Avantek	NA	NA	NA	NA	NA	NA	NA	NA	NA	Not specified	NA	NA	NA
5	Saponaro 2016 ¹⁵	CDs	48 (Same as above study)	Avantek	2	NA	NA	NA	NA	NA	NA	NA	NA	Not specified	NA	22.90 – got CD at 3 rd visit 47.92 – incorrect 47.22 – incorrect 37.5% lab reline 12.5% soft reline occlusal vertical 6.25% fracture 3.125% fracture 3.125% fracture 3.125% fracture adjustment visit 29% requiring 2 adjustment visits 13.2% for lack of denture retention 3.12 – unacceptable esthetics 122 – reported altered occlusion	0.39 extra visits 3.06 recall visits 1.06 extra visits 37.5% lab reline 12.5% soft reline occlusal vertical 6.25% fracture 3.125% fracture 3.125% fracture 3.125% fracture adjustment visit 29% requiring 2 adjustment visits 13.2% for lack of denture retention 3.12 – unacceptable esthetics 122 – reported altered occlusion
6	Schwabling 2016 ¹⁶	CD Set	20	Welland Dental Digital Denture system	4	polyvinyl siloxane monophase	Border-molded impression (no system tray)	Scanned the impression	Ivoclair centric tray, occlusal plane & gothic arch tracing	Welland system teeth arrangement (no virtual articulator)	Wax denture with acrylic resin base	Not specified	Injection mold vs. Milling	Not specified	PMMA disks (inhouse CAD for Zenoos; Welland Dental)	2 cases – insufficient OVD after preliminary RB 2 out of 5 patients have excessive lip support 1 case - excessive lip support 1 case - small buccal corridor 2 cases - teeth reposition 2 cases - teeth reposition 2 cases - problems for esthetic problems: shifting midline interpapillary line or Camper line or Camper	20% mandibular CD - loss of retention 2 out of 5 patients have excessive lip support ≥2 out of 5 patients have esthetic problem

Table 1 (Continued)

7	Bidra 2016 ¹⁷	CD Set (D&J)	40	Global Dental Science	2	No	Border-molded impression (with appliance denture)	Scanned the impression	Duplicate denture formed and added wax as necessary	Virtual tooth arrangement	No trial (if made base only)	NA	Milling	Lingualized occlusion	Press (polymerized acrylic resin in block)	Loss of retention 3-excessive wear of teeth needed for adjustment number of adjustments 2- required additional appointment	NA
8	Affeldt 2016 ¹⁸	Maxillary denture base	20	Avant	2	Alginate	Border-molded impression (with 3D printed custom tray)	Scanned the impression	No jaw registration	NA	No trial	NA	Conventional heat-activated polymerization vs. milling	NA	Not specified	NA	NA
9	AlRumayh 2018 ¹⁹	Maxillary denture base	20 (same as above study)	Avant	2	Alginate	Border-molded impression (with 3D printed custom tray)	Scanned the impression	No jaw registration	NA	No trial (denture base only)	NA	Conventional heat-activated polymerization vs. milling	NA	Not specified	NA	NA
10	Schwarz 2018 ¹⁹	CD Set	20	Ivoclar AG	4	Not specified	Border-molded precasted	Not specified	Schwarzling's protocol (using border centre tray, occlusal wax, gothic arch tracing)	Wax denture with acrylic resin base	Wax denture with acrylic resin base	NA	Milling	Not specified	NA	NA	0.6 extra visit 1.7 recall visit in first 4 weeks 2.07 for after 4 weeks 0.6% loss of retention 22.2% base loss if retention
11	Drago 2019 ¹⁰	CD Set	73	Avant	4	Preliminary border molding	Border-molded impression	Scanned the impression	Using occlusion rims over refined impression trays	NA	Milled trial denture	Clinical & Laboratory occlusion trial stage	Milling	Not specified	Not specified	NA	NA
12	Cristache 2019 ¹⁰	CDs	45	3Shape	3	Alginate	Border-molded impression	Not specified	Conventional occlusion rim on custom tray	Virtual record mounting 3Shape	NA	NA	DLP 3D printing	Not specified	0.4% TIO2-reinforced PMMA composite resin	NA	-3.06 denture retention (unscheduled visits) -2 dentures- accidentally broken and reprinted -denture in retention after 18 months
13	Srinivasan 2019 ²	Maxillary CDs CD set	12	Avant	2	NA	Master impression (border molding)	Scanned the impression	Anatomical occlusion rim on Arch Tracing	virtual record mounting teeth setup	NA	NA	Conventional vs. Milling	Not specified	Not specified	Chairside time is longer than previous studies (undergraduate dentures)	NA
14	Smith 2020 ²	CD Set	30	Ivoclar AG	4	Performed (not specified technique)	Border-molded impression	Not specified	border centre tray, occlusal plane & gothic arch tracing (as simulated 3D)	NA	3D printed trial denture	NA	Milling	Not specified	NA	NA	NA
15	Lo Russo 2020 ³²	Digital Images (impression and IOS)	-	TRIOS	-	NA	Conventional impression (with jaw model custom tray for vs. Introral scan	Introral scanning	-	NA	NA	NA	NA	NA	No definitive complete dentures	NA	NA
16	Yoon 2020 ¹⁷	Denture bases occlusion rims	-	3Shape	4	Alginate	Border-molded impression	Scanned the stone cast	Conventional occlusion rim on 3D printed baseplate	NA	NA	NA	Conventional polymerization vs. milling vs. DLP	NA	4-PMMA block (VPI -DLP printable resin (Basefil Base; Nexa Base 8 V))	NA	NA
17	Cristache 2020 ¹	CD Set (same with above)	45	exocad	2 or 3	Alginate	Border-molded impression	Scanned the impression	Gothic arch instrument set & occlusal plane (exocad software, German) facebow	Using CR virtual articulator (exocad software, German) CAD	NA	NA	DLP 3D printing	Not specified	0.4% TIO2-reinforced PMMA composite resin	NA	4.4% fracture

Table 1 (Continued)

18	Arakawa 2021 ¹	CD Set	16	Avant and Wield	2	Not specified	NA	NA	NA	Milling vs. heat-activated polymerization	Not specified	NA	NA	NA
19	Perez 2021 ²⁸	CD Set	16	Bite Denture System	2	NA	NA	NA	NA	Milling	Cutting guidance	Not specified	NA	NA
20	Stein 2021 ¹⁴	Digital Images (impressions)	-	Scanned image only	-	Alginate	Border-molded impression	Scanned the impression	No jaw registration	NA	NA	NA	NA	NA
21	Lo Russo 2021 ³³	Maxillary denture base	-	3Shape	3	NA	Border-molded impression	Intraoral scan	NA	NA	Milling vs. 3D printing	Milling-PMMA	NA	NA
22	Srinivasan 2021 ¹⁷	CD set	-	Avant	6	Alginate	Border-molded impression	Scanned wax denture	Gothic arch tracing and facebow record	Mechanical semi-adjustable articulator	Wax dentures try-in with articulator selection	NA	NA	3D printed CD - three maintenance visits (mean 1.5 months; range 1-2 months) (n=2)
23	Chaturvedi 2021 ²⁷	CD Set	45	Meshmixer software program 3.5, Autodesk, Inc., USA	Not specified	Performed (not specified specifically)	Border-molded impression	Scanned the stone cast	Using facebow and interocclusal record specified using with either occlusion rim or denture	Mechanical semi-adjustable articulator (Not specified)	NA	Polymethyl methacrylate (PMMA) blank vinyl Base Resin Denton Inc.	NA	NA
24	Dong 2021 ³⁰	CD Set	80	Hotemoff Jinn, China	3	Impression compound	Border-molded impression (with 3D printed denture)	Scanned the impression	Primary JRR - using occlusion rim and master cast by diagnostic dentures	Not specified	3D printed denture	No digital denture produced	NA	1- visit was added for digital denture 1- facial midline was inconsistent with the lip midline.
25	Elawady 2021 ³⁶	Maxillary CD & Mandibular IOD	14	3Shape	not clear	Performed (not specified specifically)	Conventional impression (not specified about border molding)	Scanned the bite record and master cast	Conventional JRR with occlusion rim	Mechanical articulator (Not specified: conventional denture)	NA	pink denture base printing resin (bestbest, Dentac 3-)	NA	NA
26	Faty 2021 ³⁵	Maxillary denture base	-	3Shape	-	Alginate	Border-molded impression	Scanned the stone cast	NA	NA	CAD-CAM vs. Conventional polymerization	Milling- Pink prepolymerized PMMA (Dentac Dental Materials)	NA	NA
27	Clark 2021 ¹	CDs	39	Avant	4	Performed (not specified)	performed	Not specified	Not specified	Not specified	Wanger Try-in	Not specified	NA	12.8% need remakes or repairs
28	Kim 2021 ³³	CDs	216	Dentac denturebase 2	-5	Alginate	Border-molded impression	Scanned the stone cast on articulator	Using occlusion rim	Using semi-adjustable articulator (Hama)	3D printed trial denture	Dentac Denture base II (printing resin) and teeth resins (Dentac Inc., Toronto, CA)	NA	>30% CD - ≥3 times recall >20% CD - remake or repair 25% pressure sore, 22% has retention problem. 3.2% occlusion 9.25% esthetic problem.
29	El Gaili 2021 ³⁴	CD Set	40	3Shape vs. exocad	maybe 4	Alginate	Conventional impression (not specified about border molding)	Scanned master cast	Using occlusion rim	Not specified	NA	Pink denture base printing resin (bestbest, Dentac 3-)	NA	NA

Table 1 (Continued)

30	Li 2022 ³⁸	Test 3D printed Denture	12	Hotamsoff Co. Ltd	-	Impression compound	Silicone impression with diagnostic loaded denture (border molding)	Scanned the impression	Primary JRR - using silicone material in first impression by diagnostic dentures	Not specified	NA	NA	3D Printing	Blateral balanced occlusion	Not specified	NA	NA
31	Ohara 2022 ⁷	CD Set	40	Not specified	3	NA	Border-molded impression (with Beata trays)	Scanned the impression	Gothic arch tracing using diagnostic impression- loaded trays	Not specified	3D printed trial denture	NA	3D printing	Not specified	Trial Denture: Dina Custom-made resin disk	Remake was reported but not clearly	Number of adjustments & time for fabrication & time for adjustment as conventional CD
32	Orake 2022 ⁴⁰	CD Set	88	3Shape	3	NA	performed border-molded impression (with dentures)	Scanned the impression	Primary JRR - using silicone material in first impression by trial dentures	NA	3D printed trial denture	Not specified	Milling	Not specified	Custom-made resin disk	NA	NA
33	Abubakar 2022 ³¹	Maxillary CDs	48	exocad	Not specified	Not specified	Not specified	Scanned the stone cast	Using occlusion rim	Mechanical articulator (BioArt A7 Dental Equipment)	3D printed trial denture	Not specified	Conventional heat-activated polymerization vs milled vs 3D printing	Not specified	Denture base printing resin (Neodent; Avadent; Dental Science BV)	NA	NA
34	El-Shahed 2022 ³³	Mandibular IODs	10	exocad	Not specified	Performed impression (specificity)	Border-molded impression	Scanned the stone cast	Using occlusion rim	Not specified	No trials	Not specified	Conventional heat-activated polymerization vs milled	Blateral balanced occlusion	gingiva-colored gingiva-activated PMMA blocks (WISSEN)	NA	NA
35	Nugur 2022 ³¹	Maxillary CDs	32	Not specified	Not specified	Not specified	performed impression	Scanned the stone cast	Using occlusion rim	Not specified	No trials	Not specified	Conventional heat-activated polymerization vs 3D printing	Not specified	NextDent denture base printing resin	NA	NA
36	Li 2022 ³⁵	Digital Images (JRR of arches of the scan of impressions)	-	Hotamsoff Co. Ltd	3	Impression compound	Border-molded impression (with 3D printed diagnostic denture)	Scanned the impression	Primary JRR - using silicone material in first impression by diagnostic dentures	Not specified	3D printed trial denture	NA	Conventional heat-activated polymerization	NA	NA	NA	NA
37	Al Hamad 2022 ³⁹	Digital Images (arch)	-	Not specified	NA	Impression compound	Border-molded impression vs. Intraoral scan	Scanned the stone cast vs. Intraoral scanning	NA	NA	NA	NA	NA	NA	NA	NA	NA
38	Maravetier 2022 ⁴⁰	Maxillary denture base	-	Avadent	4	Alginate	Border-molded impression (with 3D printed trays)	Scanned the stone cast	NA	NA	NA	NA	conventional vs. milled vs. 3D printing	NA	Denture base printing resin (Neodent; Veres-Dental BV)	NA	NA
39	Chothib 2022 ³⁵	Maxillary denture base	-	Avadent	4	Alginate	Border-molded impression (with 3D printed trays) vs. Intraoral scan	Scanned the stone cast vs. Intraoral scanning	NA	NA	NA	NA	Milling and 3D printing	NA	Denture base printing resin (Neodent; Veres-Dental BV)	NA	NA

CAD, computer-aided design; CD, complete denture; DLP, digital light processing; JRR, implant overdenture; JRR, jaws relationship recording; NA, not accessible; Not specified, performed procedure but not reported clearly.

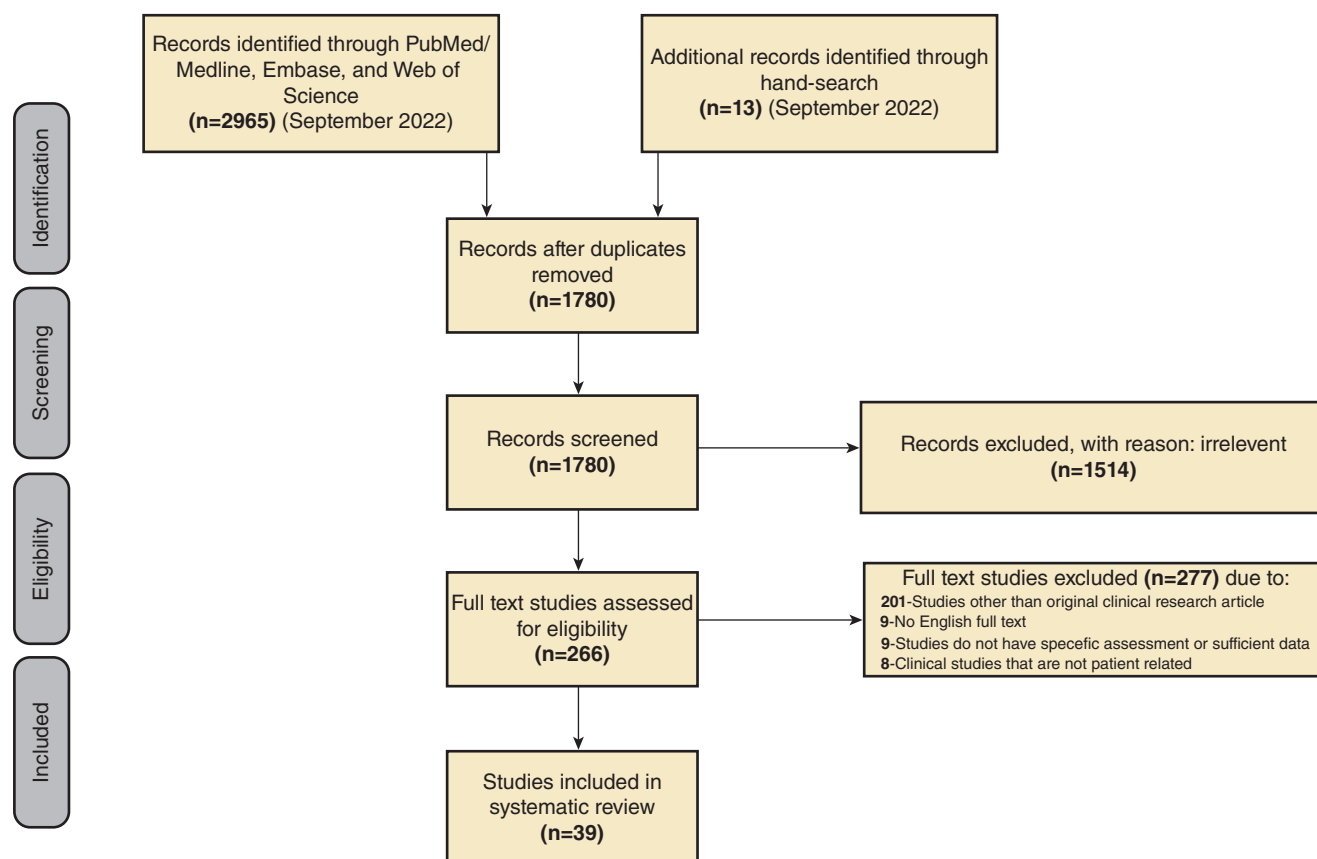


Figure 1. Preferred Reporting Items for Systematic Reviews and Meta-Analyses flowchart for screening of studies by inclusion and exclusion criteria.

trueness and/or accuracy. For studies assessing IODs,^{26,29} 1 study compared oral health-related quality of life (OHRQoL) between conventional and 3D printed IOD.²⁶ Another study investigated occlusal force and tissue surface adaptation.²⁹ For studies that assessed denture bases, 5 studies^{38,40,43-45} assessed retention, and 2 assessed accuracy.^{33,37} Details of each included study are presented in Table 1.

Thirty-four studies^{1-3,5,6,8,13-15,17-20,26-29,31,32,34-40,43-50} used the conventional impression technique, and 24^{2,3,6,13-15,17,18,20,27-29,34,35,37-40,43-48} of them also adopted border molded impression technique. Among studies using the conventional impression technique, 5 studies^{3,38,40,43,44} used CAD-CAM fabricated custom trays after primary impression making (1 milled and four 3D printed), and 1 study³² produced 3D printed custom trays after intraoral scanning. Four studies^{35,36,48,49} used 3D printed diagnostic or trial dentures as the custom trays. Fourteen studies^{3,5,15,17,18,27,28,34-36,43,44,48,49} scanned the impression to digitize the edentulous jaws, 12 studies^{20,26,29-31,37-40,45,47,50} scanned the stone casts, and 2 studies^{8,13} scanned the conventional wax trial dentures. An intraoral scanner was used to scan the edentulous jaws in 4 studies,^{32,33,38,39} but dentures were not fabricated in these studies.

In 9 studies,^{18,20,26,29-31,37,46,50} the maxillomandibular jaw relationship was recorded by using occlusion rims,

and 7 studies^{8,17,35,36,41,48,49} used existing dentures, diagnostic dentures, or their duplicates. Three studies specified the facebow record,^{13,15,47} and 7 studies used gothic arch tracing.^{2,3,5,13,15,19,27} Several commercially available digital jaw relationship record systems were found: 3 studies used the Ivoclar system (Ivoclar AG),^{2,3,19} 2 studies used the AvaDent system (Global Dental Science LLC),^{5,14} and 1 study used Baltic Denture Key system (Merz Dental GmbH).²⁸ For the Ivoclar and AvaDent systems, jaw relationship may be recorded in 2 stages. The preliminary jaw relationship was recorded with putty followed by the definitive jaw relationship recorded with trial dentures or custom trays, which might be evaluated before the definitive complete dentures are produced.^{35,36,48,49}

Six studies^{8,13,20,26,30,47} used mechanical articulators, while 2 virtual articulators, 3Shape (3Shape A/S) and exocad (exocad GmbH), were used in 2 studies.^{15,46} Four studies^{3,5,17,19} reported virtual tooth arrangement but without specifying the virtual articulator. Other studies did not report the articulator system used. Regarding the occlusal scheme of digital complete dentures, 4 studies^{13,26,29,36} used bilateral balanced occlusion, 2 studies^{14,17} used lingualized occlusion, 1 study²⁸ used canine guidance, and 1 study⁴⁷ compared 3 occlusal schemes - bilateral balanced, lingualized, and monoplane occlusions. Only 13

studies^{1-3,8,13,18-20,27,30,35,48,49} reported trial placement in the digital workflow, in which 7 studies^{2,20,27,30,35,48,49} used 3D printed and 1 study¹⁸ used milled trial dentures. Only 1 study¹⁸ reported a remount procedure.

Among the 11 CAD software programs reported, AvaDent (Global Dental Science LLC) was the most commonly used software program (12 studies^{1,5,6,13,14,16,18,38,40,42-44}), followed by 3Shape (3Shape A/S) (7 studies^{26,33,37,45,46,49,50}), exocad (exocad GmbH) (4 studies^{15,29,30,50}), Ivoclar system (Ivoclar AG) (2 studies^{2,19}), and Wieland (Wieland Dental) (2 studies^{3,6}). Twenty-one studies^{1-3,5,6,13,14,17-19,28-30,33,37,38,40,43,44,47,49} milled and 17 studies^{8,13,15,20,26,27,30,31,33,36-38,40,41,46,47,50} 3D printed the definitive complete dentures, denture bases, or trial dentures. Milling denture base materials were mainly polymethyl methacrylate (PMMA) (11 studies^{3,17,29,30,33,37,38,40,45,47,49}), while 3D printing used acrylic-based resins, including printable denture resin (12 studies^{20,26,27,30,31,33,37,38,40,45,47,50}), ultraviolet (UV) polymerized acrylic resin (2 studies^{8,41}), and titanium dioxide nanoparticle-reinforced PMMA composite resin (2 studies^{15,46}) (Table 1).

The accuracy of impression methods for digital complete dentures is summarized in Table 2. Maxillary denture bases showed the maximum discrepancy to the actual tissue surfaces (0.6 to 0.7 mm), which was measured using the thickness of the fit-checking materials.³⁷ The mean discrepancies between denture bases and stone casts or intraoral scanning or digital images of the dentures were all below 0.5 mm.^{8,29,33,38,40,50} The mean discrepancy between intraoral scanning and the conventional impression was less than 0.2 mm, while that to the stone cast was less than 0.9 mm.^{32,34,38,39,48}

A summary of the retention of digital complete dentures is listed in Table 3. The retentive force was measured in vivo with a digital force gauge in 5 studies,^{26,30,43-45} a dynamometer in 2 studies,^{38,40} and a universal testing machine in 1 study.³¹ Digital complete dentures showed better retention than conventional complete dentures.^{31,40} Most digital complete dentures have a mean retentive force of 13 to 20 N. The highest retentive force was up to 74 N among maxillary denture bases fabricated from border-molded impressions, while denture bases fabricated from intraoral scanning had the least retentive force of approximately 6 N. One study reported that the retention of maxillary denture bases fabricated from a border-molded impression (14.5 to 16.1 N) was statistically higher than those fabricated from intraoral scanning (6.2 to 6.6 N).³⁸ The retention of maxillary denture bases fabricated from a scan of definitive impressions^{43,44} was not statistically different from those fabricated from a scan of stone casts poured from definitive impressions.⁴⁵ Clinicians scored the maxillary complete dentures fabricated by milling as having better retention than that using the

injection-mold technique.³ Only 2 studies^{13,14} measured denture stability subjectively, and both found that the stability of digital complete dentures was satisfactory.

The maximum occlusal force was measured in vivo using T-scan in 1 study⁴⁷ and using an occlusal force meter in 2 studies.^{13,29} Maximum occlusal force was reported from 130 to 225 N for digital complete dentures^{13,29,47} and was similar across different fabrication procedures (Table 3).

Patients required fewer clinical visits for the fabrication of digital complete dentures than for conventional complete dentures. The preliminary impression-making and trial placement visits may be skipped, resulting in 2 to 4 fewer visits (Table 4). When compared with a conventional workflow, a reduction in clinical time (58 to 233 minutes) was specified in the fabrication of digital complete dentures than in the fabrication of conventional complete dentures.^{2,5,6,14,27,28} Digital complete dentures required statistically shorter clinical time, with 205 to 233 minutes saved in 2 studies.^{5,14} Laboratory time was reduced up to 5 hours.²⁸

In addition to the recommended number of visits, extra visits may be needed to adjust digital complete dentures (Table 5). The mean number of recall visits for postoperative review or denture adjustments were 1.0 to 4.0.^{1,13,15,18-20,27,42,48} The complications and extra visits needed are summarized in Table 5. Denture repairs or remakes were up to 31.3% of participants in 1 study.⁴² Complications with retention were found in 20.0% to 37.5% of prostheses, while other complications such as jaw relationship errors, esthetic complications, and prostheses fractures were found in less than 10.0% of prostheses.^{3,14,17-20,42} The scores of patient satisfaction and OHRQoL were similar among conventional, milled, and 3D printed complete dentures (Table 3).

DISCUSSION

Since the fabrication of digital complete dentures is relatively new, additional well-controlled clinical trials are needed to investigate the outcomes of individual procedures. This review, however, summarized the current evidence of the digital complete denture procedures and provided updated information. The research hypothesis of an association between the clinical procedures and outcomes or complications was mainly supported.

Most included studies adopted the border-molded impression technique. While intraoral scanning with border trimming has been proposed for edentulous impressions,^{32,38} the fabrication of digital complete dentures based on intraoral scanning was not common. The retention of maxillary denture bases fabricated from border-molded impressions was statistically higher than

Table 2. Clinical studies on accuracy of denture or impression and reported maximum mean values

Outcomes	Study	Comparison	Systems or Software Programs	Fabrication	Study Objects and Comparisons	Mean or Maximum Inaccuracies
Surface adaptation or Fitness or Accuracy of denture bases	Inokoshi 2012 ⁸	Wax denture vs 3D printed trial denture	3DCAD (CATIA)	3D printing	Maxillary CD	0.0051 mm
	Yoon 2020 ³⁷	Fabrication methods vs actual tissue surface of jaws (by thickness of indicator)	3Shape A/S	Milling	Mandibular CD	0.023 mm
					Maxillary denture base	0.44-0.701 mm
					Mandibular denture base	0.16-0.35 mm
					Maxillary denture base	0.31-0.59 mm
Trueness or Accuracy of impression or Intraoral scanner or Digitized models					Mandibular denture base	0.17-0.32 mm
					Maxillary denture base	0.29-0.61 mm
					Mandibular denture base	0.27-0.36 mm
	Lo Russo 2021 ³³	Fabrications vs Digital image of the corresponding designed denture base	3Shape A/S	Conventional heat-activated polymerization 3D printing	Maxillary denture base (overall accuracy)	0.002 mm
	El Galli 2021 ⁵⁰	CAD software program (definitive CD vs scanned stone cast)	3Shape vs exocad	Milling	Maxillary denture base (overall accuracy)	0.018 mm
	El-Shaheed 2022 ⁴⁹	Fabrications (Stone scan vs IOD base)	exocad	3D printing	3Shape exocad	0.09 mm
	Maniewicz 2022 ⁴⁰	Fabrications (Stone scan vs denture base)	Avadent	Milling	Mandibular IOD base (+/-)	0.25 mm
				Conventional heat-activated polymerization	Mandibular IOD base (+/-)	0.034/-0.055 mm
				Conventional heat-activated polymerization	Mandibular IOD base (+/-)	0.099/-0.081 mm
				3D printing	Maxillary denture base	0.18 mm
	Chebib 2022 ³⁸	Milled vs 3D printed denture bases vs Intraoral scan	Avadent	3D printing	Maxillary denture base	0.20-0.23 mm
	Lo Russo 2020 ³²	Maxillary and mandibular conventional impression vs IOS	Avadent	Milling	Maxillary denture base	0.21-0.23 mm
	Stein 2021 ³⁴	Selective pressure impression by various relief trays vs Control (No relief tray conventional border-molded impression) at anterior ridge and median palatal suture	Not used	3D printing	Maxillary denture base	0.21-0.22 mm
			Not used	Milling	Maxillary denture base	0.21 mm
				NA	Full scan	-0.19 mm
				NA	Trimmed scan	0.02 mm
					Control difference (both no relieves)	0.07 mm
					1 mm relief tray vs no relief	0.03 mm
					3 mm relief tray vs no relief	0.04 mm
	Deng 2021 ⁴⁸	Impression vs Denture base	Hoteamsoft Co Ltd	Conventional heat-activated polymerization	Maxillary denture base vs impression	0.165 mm
	Al Hamad 2022 ³⁹	Stone cast scan vs Intraoral scanner	Not specified	NA	Maxillary	-0.57 to 0.45 mm
	Chebib 2022 ³⁸	Intraoral scanner vs Stone cast	Avadent		Mandibular Intraoral scanner vs stone cast (root mean square)	-0.85 to 0.85 mm 0.45 mm

CD, complete denture; DLP, digital light processing; IOD, implant overdenture.

Table 3. Clinical outcomes and patient-reported outcomes of digital complete dentures

Outcomes Measured	Study	Specimens or Study Objects	Definitive Complete Dentures Fabrication Methods	Outcomes Reported
Objective retentive force measurements	AlHelal 2016 ⁴³	Maxillary denture base	Conventional heat-activated polymerization vs milling	Conventional CD base Retention (N) 54.2
	AlRumaih 2018 ⁴⁴	Maxillary denture base	Conventional heat-activated polymerization vs milling vs 3D printing	Milled CD base 74.1
	Faty 2021 ⁴⁵	Maxillary denture base	Conventional heat-activated polymerization vs milling vs 3D printing	Milled CD base 73
	Elawady 2021 ²⁶	Maxillary CD and Mandibular IOD	Conventional heat-activated polymerization vs 3D printing	3D printed CD base 68
				Baseline 3 mo 6 mo 12 mo 10.7 9.9 8.9 7
	Aboheikal 2022 ³⁰	Maxillary CD	Conventional heat-activated polymerization vs milling vs 3D printing	Milled CD ~13 ~18 ~20
	Naggar 2022 ³¹	Maxillary CD	Conventional heat-activated polymerization vs 3D-printing	3D printed CD 19.8 18.6 17.9 15.8 12.6
				Baseline 1 mo 3 mo 6 mo 9 mo 11.3 9.8 8.5 7.3 4.3
	Maniewicz 2022 ⁴⁰	Maxillary denture base	Conventional heat-activated polymerization vs milling vs 3D printing	Conventional CD base Retention (N) 10.5
	Chebib 2022 ³⁸	Maxillary denture base	Conventional border-molded impression vs intraoral scanner	Milled CD base Retention (N) 13.4 3D printed CD base 16.16.2
Subjective measurements of denture retention and stability	Kattadiyil 2015 ¹⁴	Maxillary and Mandibular CD set	Conventional heat-activated polymerization vs milling	Conventional IOS 1. Higher ratings for retention and stability by clinicians 2. Significantly higher rating for retention in maxillary arch
	Schwindling 2016 ³	Maxillary and Mandibular CD set	Milling injection molding	Retention of maxillary prostheses was rated slightly better for milled CDs
	Bidra 2016 ¹⁷	Maxillary and Mandibular CD set	Milling	(100 mm VAS, baseline → 1 y) 91.5 → 79.3 (by clinicians) 86.2 → 84.5 (by patients)
	Cristache 2019 ⁴⁶	Or CD and IOD set CD (any)	Old denture vs 3D printing	Old denture Modified Kapur Index (MKI) ≤3
				3D printed maxillary CD 7 (5-9)
	Srinivasan 2021 ¹³	CD set	Milling 3D printing	Milled CD Retention (patient' score) Stability (patient' score) Retention (Dentist' counting dentures) Stability (Dentist' counting dentures) 3.80-4.73/5 3.93-4.67/5 29/30 30/30
				3D printed CD 3.40-4.27/5 3.75-4.47/5 26/30 30/30
				3D printed mandibular CD 4 (3-5)

Table 3 (Continued)

Outcomes Measured	Study	Specimens or Study Objects	Definitive Complete Dentures Fabrication Methods	Outcomes Reported			
Masticatory performance (maximum occlusal force and chewing efficiency)	Chaturvedi 2021 ⁴⁷	5 patients	Conventional heat-activated polymerization vs milling vs 3D printing	Maximum occlusal force %	Conventional CD	Milled CD	3D printed CD
				Bilateral balance occlusion	~90	~91	~92
				Lingualized occlusion	~94	~95	95.4
	Srinivasan 2021 ¹³	15 patients	Milling vs 3D-printing	Monoplane occlusion	~81	~85	~87
				Maximum occlusal force (N)	Milled CD 154.7	3D printed CD 131.2	
				Mastication efficiency (Variance of Hue)	0.3	0.4	
PROs (patient satisfaction OHQoL and assessments)	El-Shaheed 2022 ²⁹	10 patients	Conventional heat-activated polymerization vs milling	Mastication efficiency (Subjective)	2.9	2.7	
	Inokoshi 2012 ⁸	10 patients	3D printing (Trial dentures)	Maximum occlusal force (N)	Milled IOD	Conventional IOD	
	Kattadiyil 2015 ¹⁴	15 patients	Milling	3 mo	208	166	
	Saponaro 2016 ¹⁶	50 patients	Not specified	6 mo	225	170	
					- No difference - esthetics, predictability of definitive complete dentures shape, stability, comfort of dentures, or overall satisfaction - Significantly higher patient scores for the digital CD - No significant preference on esthetics - Higher preference for digital CD for comfort, chewing efficiency, prostheses, and efficiency of the technique		
					- 78.9% - pleased with the esthetics of digital CD - 78.6% - new digital CDs were 'better' - 73.7% - satisfied with their new CDs - 68.8% - new CDs were easy to clean - 68.4% - "comfortable" and recommend to others - 57.9% - speech and chewing abilities had improved - 52.6% - fit well and stable - But no significant difference from conventional		
	Bidra 2016 ¹⁷	20 patients	Milling	79% satisfied with CAD-CAM dentures	~50% did not rate good or excellent for retention, stability, and adaptation of the bases		
	Cristache 2020 ¹⁵	35 patients	DLP 3D printing	OHIP EDENT Baseline	52.6	3D printed CD	
				12 mo	20.7		
	Peroz 2021 ²⁸	16 patients	Conventional heat-activated polymerization vs milling	OHIP G49 Baseline	20.4	Digital	
				14 d	0.3	2.7	
				3 mo	5.3	8.1	
	Elawady 2021 ²⁶	28 patients	Conventional heat-activated polymerization vs DLP 3D printing	OHIP Baseline	11.3	5.4	
				6 mo	55.9	3D printed CD 54.8	
				12 mo	49.2	39.1	
	Srinivasan 2021 ¹³	15 patients	Milling vs 3D printing	Milling	42.8	31.4	
				OHIP score	16.7	3D printed CD 26.9	
				Patient satisfaction maxillary CD	4.5	4.1	
				Patient satisfaction mandibular CD	4	3.5	
				8 patients preferred milling while 7 preferred 3D printed dentures.			

Table 3 (Continued)

Outcomes Measured	Study	Specimens or Study Objects	Definitive Complete Dentures Fabrication Methods	Outcomes Reported
	Ohara 2022 ²	20 patients	3D printing	- VAS and OHIP scores not significantly different. - VAS satisfaction ~80 to 90 for conventional CD, ~70 for digital CD - CDs >DDs for phonetics, ease of cleaning, stability, comfort, and general satisfaction VAS satisfaction 84.0 mm for digital CD and 91.0 mm for conventional CD.
	Otake 2022 ⁴	44 patients	Conventional heat-activated polymerization vs milling	Least satisfaction found in milled groups followed by conventional, while highest satisfaction found in 3D printed group.
	Aboheikal 2022 ³⁰	48 patients	Conventional heat-activated polymerization vs milling vs 3D printing	
	Maniewicz 2022 ⁴⁰	20 patients	Conventional heat-activated polymerization vs milling vs 3D printing (denture bases only)	Patients score favorably on VAS satisfaction for all CDs. Surface smoothness scored more favorably on conventional CD than on other CDs.

CD, complete denture; DLP, digital light processing; IOD, implant overdenture; OHIP, oral health impact profile; OHRQoL, oral health-related quality of life; PROs, patient reported outcomes; VAS, visual analog scale.

that of those fabricated from an intraoral scan.³⁸ Moreover, both denture wearers and clinicians rated the retention of digital complete dentures fabricated from border-molded impressions to be satisfactory.^{3,14,17} The mucocompressive nature of conventional impression-making may be responsible for the close tissue adaption and resulting improved retention.³² For intraoral scanning, the largest deviation typically occurred at the mobile mucosa,³⁹ including the soft palate, sublingual areas, and vestibule,⁵¹ important locations for the peripheral seal and retention. Furthermore, denture stability was investigated in only 2 studies by using subjective assessment.^{13,14} More studies are needed to objectively assess denture stability.

Conventional record bases with occlusion rims, existing dentures, or their duplicates, were commonly used to record the jaw relationship during digital denture fabrication.^{20,26,29-31,50} Sometimes jaw registration and definitive impression-making were performed at the same visit.^{3,15,17-19,27,36,46,48,49} In some commercially available systems, jaw relationship was recorded in 2 stages, which may allow trial placement of dentures in the second stage.

While gothic arch tracing has been specified as a standard method for recording jaw relationships in digital complete denture workflows,^{3,19} the clinical superiority of using a facebow, gothic arch tracing, and articulator in the fabrication of digital complete dentures remains unclear from this review. Occlusal relationship errors such as the improper vertical dimension of jaws and the anterior open occlusal relationship were commonly reported. These errors might be associated with imprecise jaw relationship records and a lack of trial denture placement and clinical remount steps.^{14,42} Only 13 studies performed trial denture placement, while most studies omitted this step.

Poor esthetics was a common complication,^{3,20,42} with problems that included deviated dental midlines, excessive gingival display,⁴² and unsatisfactory denture tooth and denture base shade.¹ Occlusal errors were also common. Additional visits were needed for corrections or even remaking digital dentures.^{1,3,19,42} Trial denture placement allows correction of these errors and obtaining patient approval of the esthetics. Evaluation of the digital preview of the dentures on a computer screen was found to be more difficult than a wax denture intraorally.⁵

The research hypothesis concerning the association between laboratory procedures and the outcomes of digital complete dentures was not supported. Maxillary complete dentures fabricated by milling may have better retention than those fabricated by the injection-mold technique, as rated by clinicians.³ The reason for improved retention may be related to the shrinkage-free nature of the milled PMMA.^{14,43,45} Nevertheless, the

Table 4. Clinical studies on clinical visits and chairside time in relation to steps of each commercial digital denture workflow or system

Studies	Digital Workflow					Clinical Time Difference (Saved)
	Conventional Workflow	System	Visits	Steps in Visit	Denture Fabrication	
Kattadiyil 2015 ¹⁴	5	Avadent	2	(Definitive impressions, interocclusal records, and tooth selection)+(delivery)	Not specified	205 min
Saponaro 2016 ^{16,42}	-	Avadent	2	(Definitive impressions, interocclusal records, and tooth selection)+(delivery)	Milling	-
Schwindling 2016 ³	-	Wieland Digital Denture	4	(Primary impression)+(final impression and Jaw Relationship Record)+(Try-in)+(Delivery)	Milling	-
Srinivasan 2019 ⁵	5-6	Avadent	2	(Impression, gothic arch tracing, occlusal plane orientation+tooth size) and (delivery)	Milling	233 min
Smith 2020 ²	5	Ivoclar AG	4	(Primary impression)+(final impression and gothic arch tracing)+(Try-in)+(Delivery)	3D printing and milling	60 min
Arakawa 2021 ⁶	Not specified	Avadent and Wieland	Avadent-2, Wieland-4	Not specified in detail	Milling	77 min
Clark 2021 ¹	5	Wagner Try-in workflow from Avadent	4	(Preliminary impressions)+(Definitive Impressions)+(Wagner Try-in)+(Delivery)	Milling	-
Peroz 2021 ²⁸	5	Baltic Denture System	2	(Individualization of the maxillary Baltic Denture (BD) Key and adjustment with the BD Plane+Definitive maxillary impression [silicone]+Individualization of the mandibular BD Key+Definitive mandibular impression [silicone])+(Delivery)	Milling	58 min (320 min for lab)
Deng 2021 ⁴⁸	5	Hoteamsoft Co Ltd	3	(Primary impression+Jaw relation record)+(definitive impression+definitive jaws relation record+esthetic try-in with diagnostic denture)+(Delivery)	Heat-activated polymerization	-
Ohara 2022 ²⁷	5	Not specified	3	(Definitive impression+Jaw relation record+gothic arch tracing)+(Try-in)+(Delivery)	3D printing	2.2 h (no difference)

Table 5. Clinical studies investigating common complications and extra visits for digital complete dentures in relation to fabrication steps

Studies	Digital Systems	Visits	Trial Denture Placement	Definitive Complete Dentures Fabrication	Extra Visit Needed	Recall Visit for Complaints or Post Insertion	Remake or Repair	Pressure Sore	Loss of Retention or Need to Reline or Border Modification	Vertical Dimension or Occlusal Relationship Errors	Esthetic Complications	Fracture
Kattadiyil 2015 ¹⁴	Avadent	2	No Try-in	Not specified	-	-	-	-	-	6.6% of patients (anterior open relation)	-	-
Schwindling 2016 ³	Wieland Digital Denture	4	Performed Try-in	Milling Injection Molding	1.4	-	-	-	20% mandibular denture 37.5% (lab reline) 12.5% (soft reline)	2 out of 5 patients	≥2 out of 5 patients	-
Saponaro 2016 ^{16,42}	Avadent	2	No Try-in	Milling	0.4	2.1	31.3%	Main reason for increasing recall visits	1	-	-	6.25%
Bidra 2016 ¹⁷					2 participants – additional visits 0.6	-	-	-	-	-	-	-
Schlenz 2018 ¹⁹	Ivoclar AG	4	Performed Try-in	Milling		1.7 for first 4 wk 2.07 for after 4 wk		61.0%-66.7% of follow up	20%-22.2% of follow-up (for reline)	5.6% of follow up	-	5.6%-6.7% of follow up
Drago 2019 ¹⁸	Avadent	4	Performed Try-in	Milling	-	1	Not specified		Not specified	Not specified	Not specified	Not specified 2 dentures
Cristache 2019 ⁴⁶	3Shape	2 or 3	No Try-in	DLP 3D printing		3.1			A reduction of retention after 18 mo			4.4% of digital dentures 2-in 3D printed dentures
Cristache 2020 ¹⁵	exocad	3	No Try-in	DLP 3D printing	-	-	-	-	-	-	-	
Srinivasan 2021 ¹³	Avadent	6	Wax dentures try-in	Milling vs 3D printing	-	3D printed denture: 3 (planned visit=1, unscheduled visit=2) (Total adjust-ments Milling Denture-26 3D printed denture-40)	1: in 3D printed denture	-	-	-	-	
Deng 2021 ⁴⁸	Hoteamsoft Co Ltd	3	3D printed trial denture	Conventional heat-activated polymerization	1 patient needs an extra visit	1.6 in student-treated groups 1.2 in physicians-treated groups	1- remake			1-unstable jaw relation	1-facial midline inconsistent with lip midline 2-highly required esthetic adjustment	

Table 5 (Continued)

Studies	Digital Systems	Visits	Trial Denture Placement	Definitive Complete Dentures Fabrication	Extra Visit Needed	Recall Visit for Complaints or Post Insertion	Remake or Repair	Pressure Sore	Loss of Retention or Need to Reline or Border Modification	Vertical Dimension or Occlusal Relationship Errors	Esthetic Complications	Fracture
Kim 2021 ²⁰	Dentica denture base 2	5	Performed Try-in	3D printing	-	≥3 times - ~20% of maxillary CD ~29% of mandibular CD	28% maxillary CD 32% mandibular CD	35%	22% 2.7% stability	3.2% in occlusion	9.3%	-
Clark 2021 ¹	Wagner Try-in workflow from	4	Performed Try-in	Milling	5% need additional ≥2 visits	1-2 out of 3 recalls	12.8% of digital dentures	-	-	-	-	-
Ohara 2022 ²⁷	Avadent Not specified	3	3D printed denture Try-in	3D printing	~1 visit	~4 (4000 seconds)	-	-	-	-	-	-

CD, complete denture; DLP, digital light processing.

objective retention of milled complete dentures was not significantly different from that of 3D printed ones.^{30,31,38,40,43,45} No superiority was specified among different fabrication techniques in most clinical and patient-reported outcomes, nor in the frequency of follow-up visits¹⁸ or patient and clinician preference. However, the 3D printed complete dentures are less expensive in terms of material costs and fabrication time than milled complete dentures.² The 3D printing technology has mainly been used to fabricate trial dentures, but the development of materials and technology has now allowed the fabrication of definitive complete dentures offering outcomes comparable with those of milled dentures.¹³

Digital dentures required around one-third of the time needed for the fabrication of conventional dentures.²⁸ Clinical steps can be combined to save clinical time,^{5,6,14,28} and the laboratory worktime was also much reduced.²⁸ However, extra visits may be needed because patients or clinicians may be dissatisfied with the definitive digital complete dentures. The most common complaints about digital complete dentures were pain and pressure spots,^{19,20,42} common complications in all removable dentures.⁵² In addition, occlusal relationship errors,^{3,8,14,16} lack of denture retention,^{19,42} and poor esthetics³ were prevalent complications that required extra visits (Table 5). After delivery of the definitive complete dentures, up to 4 visits may be needed for corrections or adjustments. However, digital complete dentures have been reported^{1,18} to require fewer follow-up visits and fewer numbers of denture adjustments than conventional complete dentures.^{18,20} The basic requirement of complete dentures persists, and attention to impression-making, jaw relationship recording, and esthetic parameters is key to denture success. Limitations of this systematic review included that some studies were rated as poor in quality. Moreover, heterogeneity was observed in both the study design and the investigated denture specimens. Therefore, caution must be exercised when extrapolating the results of this review to clinical practice.

CONCLUSIONS

Based on the findings of this systematic review, the following conclusions were drawn.

1. Border-molded impression-making for recording functional denture borders is preferred for improved retention of digital complete dentures when compared with intraoral scanning.
2. Correct jaw relationship records and trial denture placement are essential in the digital denture workflow to prevent esthetic and occlusal complications. Gothic arch tracing and facebow transfer can be used to obtain accurate jaw relationship records.

3. Fabrication techniques for digital complete dentures, either milling or 3D printing, do not influence patient satisfaction, preference, or OHRQoL outcomes.

APPENDIX A. SUPPORTING INFORMATION

Supplemental data associated with this article can be found in the online version at [doi:10.1016/j.prosdent.2023.07.027](https://doi.org/10.1016/j.prosdent.2023.07.027).

REFERENCES

1. Clark WA, Brazile B, Matthews D, Solares J, De Kok JJ. A comparison of conventionally versus digitally fabricated denture outcomes in a university dental clinic. *J Prosthodont*. 2021;30:47–50.
2. Smith PB, Perry J, Elza W. Economic and clinical impact of digitally produced dentures. *J Prosthodont*. 2021;30:108–112.
3. Schwindling FS, Stober T. A comparison of two digital techniques for the fabrication of complete removable dental prostheses: A pilot clinical study. *J Prosthet Dent*. 2016;116:756–763.
4. Srinivasan M, Kamnoedboon P, McKenna G, et al. CAD-CAM removable complete dentures: A systematic review and meta-analysis of trueness of fit, biocompatibility, mechanical properties, surface characteristics, color stability, time-cost analysis, clinical and patient-reported outcomes. *J Dent*. 2021;113:103777.
5. Srinivasan M, Schimmel M, Naharro M, O' Neill C, McKenna G, Müller F. CAD/CAM milled removable complete dentures: Time and cost estimation study. *J Dent*. 2019;80:75–79.
6. Arakawa I, Al-Haj Husain N, Srinivasan M, Maniewicz S, Abou-Ayash S, Schimmel M. Clinical outcomes and costs of conventional and digital complete dentures in a university clinic: A retrospective study. *J Prosthet Dent*. 2022;128:390–395.
7. Maeda Y, Minoura M, Tsutsumi S, Okada M, Nokubi T. A CAD/CAM system for removable denture. Part I: Fabrication of complete dentures. *Int J Prosthodont*. 1994;7:17–21.
8. Inokoshi M, Kanazawa M, Minakuchi S. Evaluation of a complete denture trial method applying rapid prototyping. *Dent Mater J*. 2012;31:40–46.
9. Kanazawa M, Inokoshi M, Minakuchi S, Ohbayashi N. Trial of a CAD/CAM system for fabricating complete dentures. *Dent Mater J*. 2011;30:93–96.
10. Kanazawa M, Iwaki M, Arakida T, Minakuchi S. Digital impression and jaw relation record for the fabrication of CAD/CAM custom tray. *J Prosthodont Res*. 2018;62:509–513.
11. Lam WYH, Hsung RTC, Choi WWS, Luk HWK, Pow EHN. A 2-part facebow for CAD-CAM dentistry. *J Prosthet Dent*. 2016;116:843–847.
12. Lam WYH, Hsung RTC, Choi WWS, Luk HWK, Cheng LYY, Pow EHN. A clinical technique for virtual articulator mounting with natural head position by using calibrated stereophotogrammetry. *J Prosthet Dent*. 2018;119:902–908.
13. Srinivasan M, Kalberer N, Fankhauser N, Naharro M, Maniewicz S, Müller F. CAD-CAM complete removable dental prostheses: A double-blind, randomized, crossover clinical trial evaluating milled and 3D printed dentures. *J Dent*. 2021;115:103842.
14. Kattadiyil MT, Jekki R, Goodacre CJ, Baba NZ. Comparison of treatment outcomes in digital and conventional complete removable dental prosthesis fabrications in a predoctoral setting. *J Prosthet Dent*. 2015;114:818–825.
15. Cristache CM, Totu EE, Iorgulescu G, et al. Eighteen months follow-up with patient-centered outcomes assessment of complete dentures manufactured using a hybrid nanocomposite and additive CAD/CAM protocol. *J Clin Med*. 2020;9:324.
16. Saponaro PC, Yilmaz B, Johnston W, Heshmati RH, McGlumphy EA. Evaluation of patient experience and satisfaction with CAD-CAM-fabricated complete dentures: A retrospective survey study. *J Prosthet Dent*. 2016;116:524–528.
17. Bidra AS, Farrell K, Burnham D, Dhingra A, Taylor TD, Kuo CLL. Prospective cohort pilot study of 2-visit CAD/CAM monolithic complete dentures and implant-retained overdentures: Clinical and patient-centered outcomes. *J Prosthet Dent*. 2016;115:578–586.
18. Drago C, Borgert AJ. Comparison of nonscheduled, postinsertion adjustment visits for complete dentures fabricated with conventional and CAD-CAM protocols: A clinical study. *J Prosthet Dent*. 2019;122:459–466.
19. Schlenz MA, Schmidt A, Wöstmann B, Rehmann P. Clinical performance of computer-engineered complete dentures: A retrospective pilot study. *Quintessence Int*. 2019;50:706–711.
20. Kim TH, Huh JB, Lee J, Bin EB, Park CJ. Retrospective comparison of postinsertion maintenances between conventional and 3D printed complete dentures fabricated in a predoctoral clinic. *J Prosthodont*. 2021;30:158–162.
21. Kattadiyil MT, AlHelal A, Goodacre BJ. Clinical complications and quality assessments with computer-engineered complete dentures: A systematic review. *J Prosthet Dent*. 2017;117:721–728.
22. Kattadiyil MT, AlHelal A. An update on computer-engineered complete dentures: A systematic review of clinical outcomes. *J Prosthet Dent*. 2017;117:478–485.
23. Bidra AS, Taylor TD, Agar JR. Computer-aided technology for fabricating complete dentures: Systematic review of historical background, current status, and future perspectives. *J Prosthet Dent*. 2013;109:361–366.
24. Rasaie V, Abduo J. Current techniques for digital complete denture fabrication. *Int J Comput Dent*. 2022;25:181–199.
25. Page MJ, Moher D, Bossuyt PM, et al. PRISMA 2020 explanation and elaboration: Updated guidance and exemplars for reporting systematic reviews. *BMJ*. 2021;372:n160.
26. Elawady DM, Ibrahim WI, Osman RB. Clinical evaluation of implant overdentures fabricated using 3D-printing technology versus conventional fabrication techniques: A randomized clinical trial. *Int J Comput Dent*. 2021;24:375–384.
27. Ohara K, Isshiki Y, Hoshi N, et al. Patient satisfaction with conventional dentures vs. digital dentures fabricated using 3D-printing: A randomized crossover trial. *J Prosthodont Res*. 2022;66:623–629.
28. Peroz S, Peroz I, Beuer F, Sterzenbach G, von Stein-Lausnitz M. Digital versus conventional complete dentures: A randomized, controlled, blinded study. *J Prosthet Dent*. 2022;128:956–963.
29. El-Shaheed NH, Lamfon HA, Salama RI, Faramawy AMG, Mostafa AZH. Tissue surface adaptation and clinical performance of CAD-CAM milled versus conventional implant-assisted mandibular overdenture. *Int J Dent*. 2022:8220233.
30. Aboheikal MM, Nabi NA, Elkerdawy MW. A study comparing patient satisfaction and retention of CAD/CAM milled complete dentures and 3D printed CAD/CAM complete dentures versus conventional complete dentures: A randomized clinical trial. *Braz Dent Sci*. 2022;25:1–11.
31. Naggar SMEL, Helal E, Khalil MFF, El-sisy AME, Gouda A. Comparative study of maxillary denture-base retention between CAD/CAM (3D printed) and conventional fabrication techniques: A randomized clinical study. *J Arab Soc Med Res*. 2022;17:46–51.
32. Lo Russo L, Caradonna G, Troiano G, Salamini A, Guida L, Ciavarella D. Three-dimensional differences between intraoral scans and conventional impressions of edentulous jaws: A clinical study. *J Prosthet Dent*. 2020;123:264–268.
33. Lo Russo L, Guida L, Zhurakivska K, Troiano G, Chochlidakis K, Ercoli C. Intaglio surface trueness of milled and 3D printed digital maxillary and mandibular dentures: A clinical study. *J Prosthet Dent*. 2023;129:131–139.
34. Stein BE, Yoon HI, Mattie H, Lee SJ. Quantitative analysis of the selective pressure impression technique using CAD-CAM technology: A pilot clinical study. *J Prosthet Dent*. 2022;128:1289–1294.
35. Li W, Chen H, Wang Y, Xie Q, Sun Y. Digital determination and recording of edentulous maxillomandibular relationship using a jaw movement tracking system. *J Prosthodont*. 2022;31:663–672.
36. Li W, Xie Q, Wang Y, Sun Y. Quantitative evaluation of edentulous maxillomandibular relationship record using diagnostic complete dentures fabricated by CAD and 3D printing. *J Oral Sci*. 2022;64:59–62.
37. Yoon SN, Oh KC, Lee SJ, Han JS, Yoon HI. Tissue surface adaptation of CAD-CAM maxillary and mandibular complete denture bases manufactured by digital light processing: A clinical study. *J Prosthet Dent*. 2020;124:682–689.
38. Chebib N, Imamura Y, El Osta N, Srinivasan M, Müller F, Maniewicz S. Fit and retention of complete denture bases: Part II – conventional impressions versus digital scans: A clinical controlled crossover study. *J Prosthet Dent*. 2022.
39. Al Hamad KQ, Al-Kaff FT. Trueness of intraoral scanning of edentulous arches: A comparative clinical study. *J Prosthodont*. 2023;32:26–31.
40. Maniewicz S, Imamura Y, El Osta N, Srinivasan M, Müller F, Chebib N. Fit and retention of complete denture bases: Part I – Conventional versus CAD-CAM methods: A clinical controlled crossover study. *J Prosthet Dent*. 2022.
41. Katase H, Kanazawa M, Inokoshi M, Minakuchi S. Face simulation system for complete dentures by applying rapid prototyping. *J Prosthet Dent*. 2013;109:353–360.
42. Saponaro PC, Yilmaz B, Heshmati RH, McGlumphy EA. Clinical performance of CAD-CAM-fabricated complete dentures: A cross-sectional study. *J Prosthet Dent*. 2016;116:431–435.
43. AlHelal A, AlRumaih HS, Kattadiyil MT, Baba NZ, Goodacre CJ. Comparison of retention between maxillary milled and conventional denture bases: A clinical study. *J Prosthet Dent*. 2017;117:233–238.

44. AlRumaih HS, AlHelal A, Baba NZ, Goodacre CJ, Al-Qahtani A, Kattadiyil MT. Effects of denture adhesive on the retention of milled and heat-activated maxillary denture bases: A clinical study. *J Prosthet Dent*. 2018;120:361–366.
45. Faty M, Sabet M, Thabet Y. A comparison of denture base retention and adaptation between CAD-CAM and conventional fabrication techniques. *Int J Prosthodont* 2022.
46. Cristache CM, Totu EE, Grosu AR, Ene O, Beuran IA, Burlibasa M. Nanocomposite for rapid prototyped complete denture eighteen months follow-up on clinical performance. *Rev Chim*. 2019;70:387–392.
47. Chaturvedi S, Addas MK, Alqahtani NM, Al Ahmari NM, Alfarsi MA. Clinical analysis of CAD-CAM milled and printed complete dentures using computerized occlusal force analyser. *Technol Health Care*. 2021;29:797–811.
48. Deng K, Chen H, Wang Y, Zhou Y, Sun Y. Evaluation of functional suitable digital complete denture system based on 3D printing technology. *J Adv Prosthodont*. 2021;13:361–372.
49. Otake R, Kanazawa M, Iwaki M, et al. Patient-reported outcome and cost-effectiveness analysis of milled and conventionally fabricated complete dentures in a university clinic: A retrospective study. *J Prosthet Dent* 2022.
50. El Galil EGA, Mohamed S, Rizk F, Sabet M. Evaluation of two computer-aided design software on the adaptation of digitally constructed maxillary complete denture. *J Indian Prosthodont Soc*. 2021;21:383–390.
51. Hack G, Liberman L, Vach K, Tchorz JP, Kohal RJ, Patzelt SBM. Computerized optical impression making of edentulous jaws – An in vivo feasibility study. *J Prosthodont Res*. 2020;64:444–453.
52. Bilhan H, Erdogan O, Ergin S, Celik M, Ates G. Complication rates and patient satisfaction with removable dentures. *J Adv Prosthodont*. 2012;4:109–115.

Corresponding author:

Dr Walter Yu Hang Lam
Faculty of Dentistry
The University of Hong Kong
Prince Philip Dental Hospital
3B18
34 Hospital Road
Sai Ying Pun, Hong Kong
CHINA
Email: retlaw@hku.hk.

CRediT authorship contribution statement

Khaing Myat Thu: Conceptualization, Methodology, Software, Formal analysis, Investigation, Resources, Data curation, Writing - original draft, Writing - review and editing, Visualization. **Pedro Molinero-Mourelle:** Conceptualization, Methodology, Software, Formal analysis, Investigation, Resources, Data curation, Writing - review and editing, Visualization. **Andy Wai Kan Yeung:** Conceptualization, Methodology, Validation, Writing - review and editing, Supervision. **Samir Abou-Ayash:** Methodology, Writing - review and editing, Supervision. **Walter Yu Hang Lam:** Conceptualization, Methodology, Validation, Resources, Writing - review and editing, Supervision, Project administration.

Copyright © 2024 The Authors. Published by Elsevier Inc. on behalf of the Editorial Council of *The Journal of Prosthetic Dentistry*. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>). <https://doi.org/10.1016/j.prosdent.2023.07.027>